

**Scope of accreditation of research laboratory
No AB 120
issued by Polish Centre for Accreditation Issue
No. 17 of 12 June 2019.**

Head of the laboratory

The experts

Grażyna Kulesza, PhD, Eng.
g.kulesza@imim.pl

Marek Lipiński, PhD, DSc

Zbigniew Starowicz, PhD, Eng

Address:

**Institute of Metallurgy and Materials Science Polish
Academy of Sciences**

ul. Reymont 25, 30-059 Krakow

phone: (48) 12 295 28 98, fax: (48) 12 295 28 04

e-mail: zlb@imim.pl, website: <http://www.imim.pl>

Photovoltaic Laboratory

22 Krakowska St. PL-43340 Kozy

phone: (48) 33 817 4249

Apparatus:

Module Solar Simulator

Series: Quick Sun 820A, Producer: Endecas Oy

The simulator is designed to measure current-voltage characteristics and the resulting electrical parameters of PV modules. This device consists of a high quality light source in the form of flash Xenon Lamp, which allows illuminating the module with the light similar to the sunlight during the measurement. This lamp is supplied with flash generators, which transfer the energy appropriate to the research carried

out under the STC (Standard Test Conditions). Moreover, simulator is equipped with a central processing unit allowing the flash control and data acquisition. The Endeas software is responsible for processing the data obtained during the measurement. Additionally, the entire device is equipped with a special test frame for conducting measurements in total blackout and infrared sensor for non-contact temperature measurement module.

The individual components of the measurement system are shown schematically in Fig. 1.

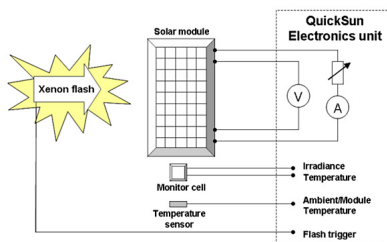


Fig. 1. The scheme of the measurement system - simulator for the measurement of PV modules electrical parameters.

During the module measurements, the connection based on the 4-probes measurement principle is used, what allows to measure correctly the electrical parameters of PV modules without loss of power associated with the resistance of the cables and connectors.

Complete current-voltage characteristics are obtained after one flash at a given radiation intensity level when the module is connected to the measurement circuit. It is possible to carry out the tests under STC (1000 W/m^2), and for any radiation power in the range $200\text{-}1000 \text{ W/m}^2$ for the spectrum of AM 1.5.

The results are presented in a graphical and numerical form. Numerically determined are:

ISC - short circuit current,
IMP - current in the maximum power point,
VOC - open circuit voltage,
VMP - voltage in the maximum power point,
PM - maximum power,
FF - fill factor,
Eff - photovoltaic conversion efficiency.

In addition, there are numerically determined parameters such as:

RS - series resistance
RSH - shunt resistance

Numerical and graphical measurement result is shown in Fig. 2.

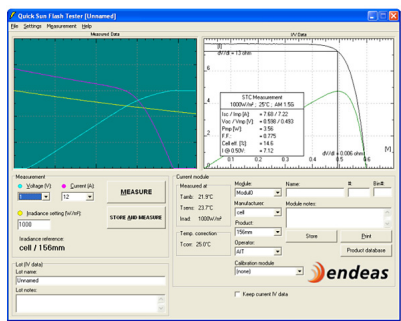


Fig. 2. The window depicting the result of the module measurement.

Solar simulator works in measurement class of AAAA determined in accordance with IEC 60904-09, ed. 2. Basic technical parameters of the simulator and AAAA class consisting parameters are shown in Table 1

Table 1. Quick Sun 820A simulator parameters

Parameter	Value (testing class)
-----------	-----------------------

Max. module size	200cmx20m]
No. measurement	120
Over time of 1 h	

Measurement cell size [cm x cm]

Lamp pulse duration [ms]

Radiation intensity [W/m^2]

Lamp lifetime [h]

□ **Spectrum** $< \pm 25\%$

□ **Non-Uniformity (NU)** $\pm 2\%$

□ **Short term instability (STI)** $< 0,5\%$

□ **Long term instability (LTI)** $< \pm 2\%$

Preparation of tested samples:

The measurement is acceptable for the photovoltaic modules made of monocrystalline, polycrystalline silicon and thin-film amorphous silicon as well.

The laboratory performs tests on PV modules supplied by the customer. During the reconciliation of the order conditions the customer is informed about the requirements for the modules and how they should be prepared for the tests.

Photovoltaic module for testing should have dimensions not exceeding 200 x 120 cm.

Solar Simulator with the system for I-V characteristic measurements of solar cells

Solar Simulator: Model SS 200AAA

Producer: Photo Emission Tech Inc.

System for I-V characteristic measurements of solar cells: „Solar cell I-V curve tracer" model SS I-V CT-02" with the Auxiliary Unit ver.2

Producer: PV Test Solutions Tadeusz Żdanowicz

Solar Cells Simulator with the I-V characteristics measurement system is designed for the measurements of current-voltage characteristics in the STC (Standard Test Conditions) defined by European standard IEC 60904-3 as irradiance with spectrum corresponding to AM1.5 (G means global) equal to 1000 W/m² and cell temperature 25 °C and NOCT (Nominal Operating Cell Temperature Conditions according to the IEC 61853-1) conditions respectively. System for I-V characteristic measurements of solar cells meets all requirements of the IEC 60904-1 standard. The all components of the system are presented in Fig. 3 - 5.

Used four probes (Kelvin) technique is necessary to correct measurement of the electrical parameters of solar cells without power losses associated with the resistance of the cables and connectors. This means that two separate probes are needed

to electrical current flow through the cell while other two are used to directly measure voltage drop on the cell. In this system brass plate with polished and gold plated surface serves as the back current probe. Inside the table, in its central part, two voltage gold plated probes for solar cell back-side contacting are located. These probes are electrically isolated from the table. Contacting to solar cell's front side is provided by the set of four coupled voltage/current gold-plated telescopic probes. Additionally, also another probing option is used. This is a system with two or three sets of multi-pin soft-touch gold plated probes mounted to the aluminium frame (Fig.4). This system is suitable for testing large amount of big solar cells ($\geq 16,5 \times 16,5$ cm).

A Heating-Cooling Controller has been designed to control the temperature of the measuring table in the range of $\sim 0-60$ °C. This is done by supplying electrical current to set of four Peltier elements having total maximum rated power of about 280 W. The elements have been attached to the rear side of the measuring table. Depending on the direction of the current through Peltier elements the table may be either heated or cooled.

This I-V measurement system measures I-V curves of solar cells both in dark as well in light mode. Light I-V characteristics are registered under stable light of specified intensity.

Numerical and graphical measurement result is shown in Fig. 5.

The result of the measurement is characteristic I-V in a graphical and in standard text (ASCII) file, and set of numerical data and cell parameters:

ISC - short circuit current,
IMP - current in the maximum power point,
VOC - open circuit voltage,
VMP - voltage in the maximum power point,
PM - maximum power,
FF - fill factor,
Eff - photovoltaic conversion efficiency.

In addition, there are numerically determined parameters such as:

RS - series resistance
RSH - shunt resistance

To determine

In order to accurately determine the series resistance, the

procedure described in the standard IEC60891 has been applied. This procedure requires measurement of the two I-V curves under two significantly different light intensities.

Additionally, data I-V may be subjected to additional analysis by fitting I-V curve to specified cell's equivalent diode model (SEM, DEM or VDEM).

The result is a diode parameters such as dark current density, diode quality factor, series and parallel resistance.

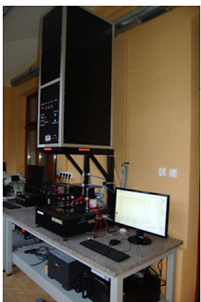


Fig. 3. The view of the setup for measurement I-V characteristics of solar cells

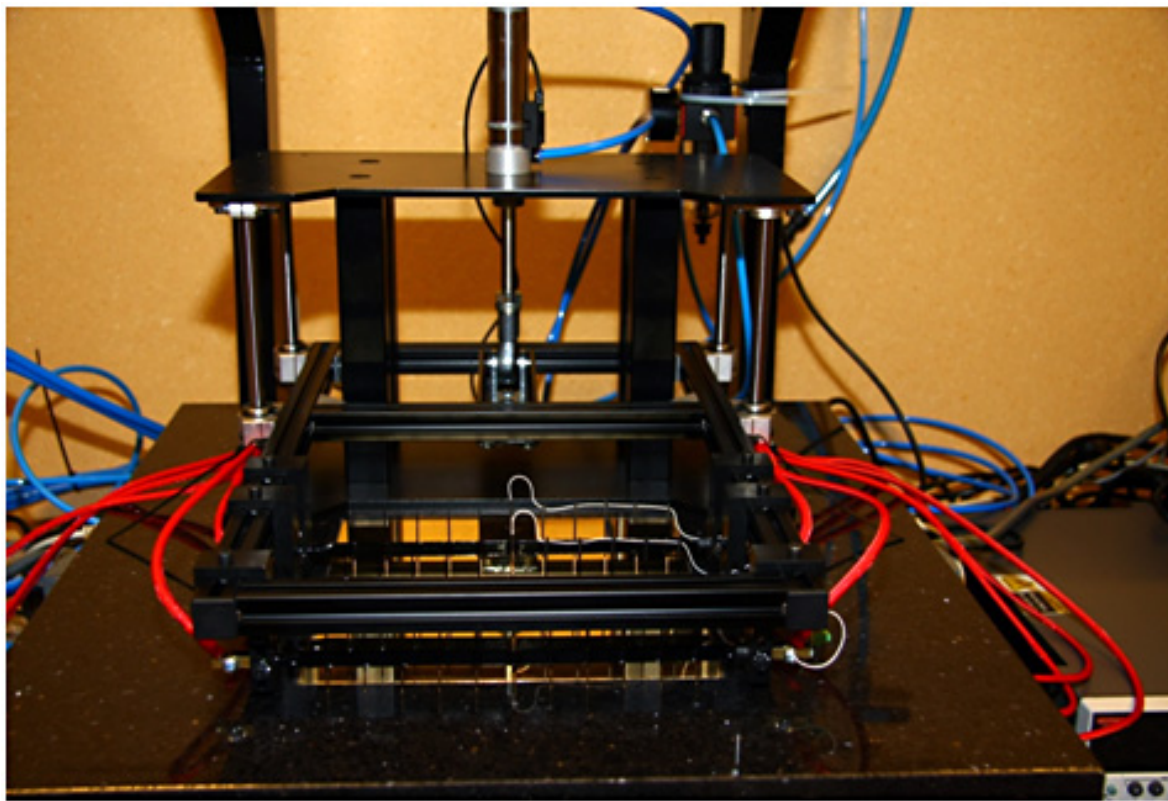


Fig. 4. Measuring table with the multi-pin voltage/current probes of the setup (Fig.3).






Spectrophotometer UV-VIS-NIR

Series: Lambda 950 S

Producer: Perkin Elmer

Spectrophotometer Lambda 950 S (Fig. 7) is designed for optical parameters measurements especially: reflectance, transmission coefficient in the solid and liquid materials in the wavelength range of 200 - 2500 nm.

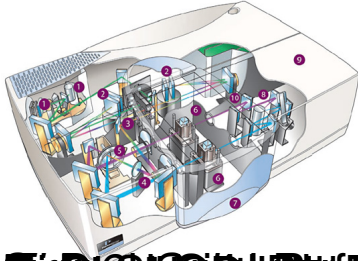

Head of the laboratory L-9:

Prof. Marek Lipiński, PhD, DSc.

tel: 33 817 42 49 e-mail: m.lipinski@imim.pl or marlipin@wp.pl

PCA

Zakre

Laboratorium Fotowoltaiczne w Kozach L-9 ul. Krakowska 22; 43-340 Kozy		
Przedmiot badań/wyrób	Rodzaj działalności/ badane cechy/metoda	Dokumen
Moduły fotowoltaiczne na bazie ogniw z krzemu mono i polikrystalicznego oraz z krzemu amorficznego	Parametry elektryczne i charakterystyki prądowo-napięciowe ogniw fotowoltaicznych Wielkość badanego ogniwa Zakres: (20x20 – 200x200) mm Napięcie ogniwa Zakres: (0 – 2,5) V Prąd ogniwa Zakres: (0 – 20) A Pomiar z użyciem symulatora promieniowania słonecznego oraz układu pomiarowego (dla warunków STC)	P/19/IB-20 wyd. 2 zmod. 24
Moduły fotowoltaiczne^E	Parametry elektryczne i charakterystyki prądowo-napięciowe modułów fotowoltaicznych Pomiar z użyciem symulatora promieniowania słonecznego oraz układu pomiarowego	P/19/IB-18
Materiały lite i ciekłe^E	Absorbancja i współczynniki odbicia i transmisji światła Metoda spektrofotometryczna	P/19/IB-19

E – Elastyczny zakres akredytacji. Elastyczność zakresu obejmuje elementy wskazane w dokumencie DA-10 laboratoriów badawczych.

Lista działań prowadzonych w ramach elastycznego zakresu akredytacji jest udostępniana publicznie lub na żądanie akredytowany podmiot.

Laboratorium formułuje opinie i interpretacje w sprawozdaniach z badań podanych w powyższej tabeli.

